




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61M 16/08, A61B 5/08	A1	(11) International Publication Number: WO 00/45884 (43) International Publication Date: 10 August 2000 (10.08.00)
(21) International Application Number: PCT/SE00/00113 (22) International Filing Date: 20 January 2000 (20.01.00) (30) Priority Data: 9900351-9 2 February 1999 (02.02.99) SE (71) Applicant (for all designated States except US): ARTEMA MEDICAL AB [SE/SE]; Rissneleden 136, S-174 57 Sundbyberg (SE). (72) Inventors; and (75) Inventors/Applicants (for US only): ECKERBOM, Anders [SE/SE]; Pl 669, S-185 41 Vaxholm (SE). LINDESTAM, Per [SE/SE]; Bolindervägen 113, S-176 54 Järfälla (SE). (74) Agents: KARLSTRÖM, Lennart et al.; Noréns Patentbyrå AB, Box 10198, S-100 55 Stockholm (SE).		(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments. In English translation (filed in Swedish).

(54) Title: LIQUID SEPARATOR WITH HOLDER UNIT

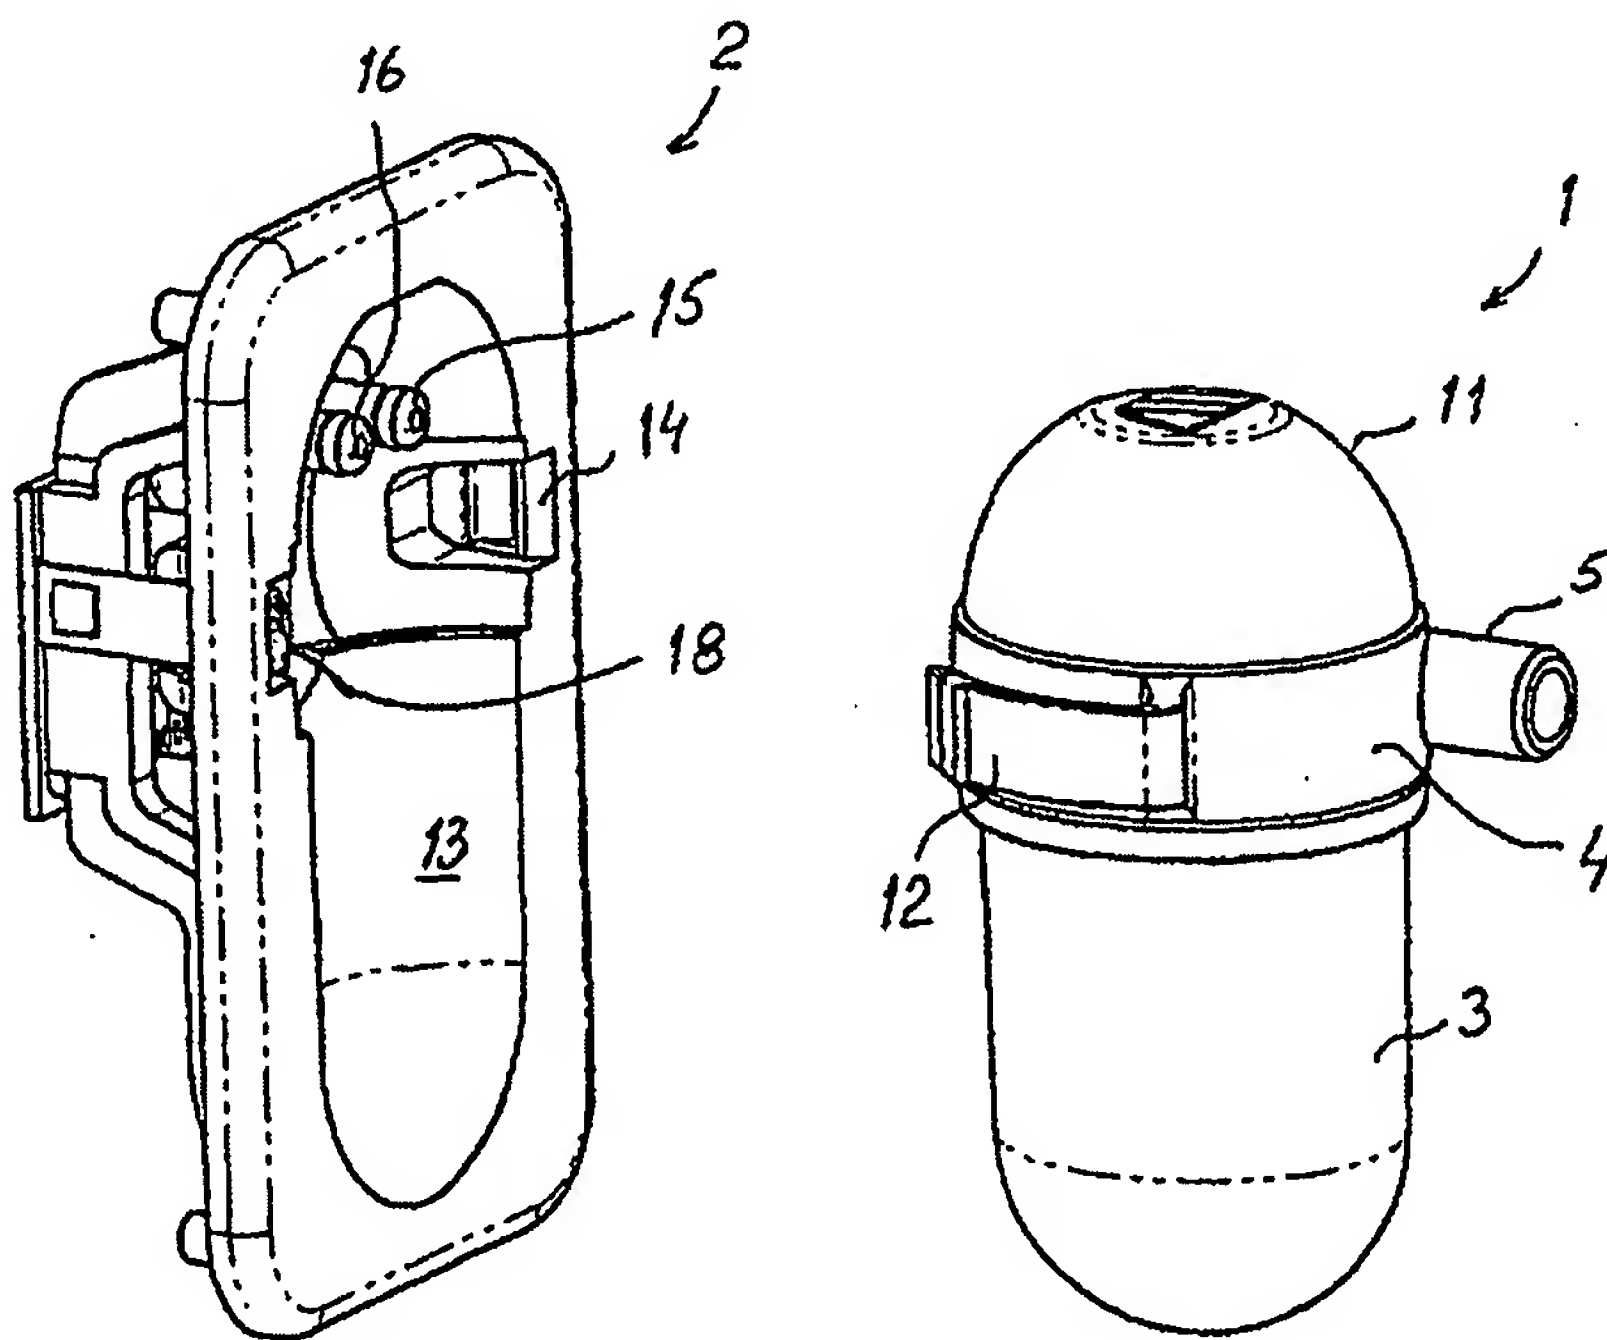

(57) Abstract

The present invention relates to a liquid separator for separating liquid from gases, comprising a water trap (1) that includes a container (5), a connector (5) for incoming gas flow, a separation chamber (4) that includes a filter and at least one connection passageway for leading separated gas to an analysis instrument, wherein the water trap (1) can be removably fitted in a holder unit (2) connected to the analysis instrument, and wherein the holder unit (2) includes connection devices (15, 16) for receiving the connection passageway.

LIQUID SEPARATOR WITH HOLDER UNIT

The present invention relates to a liquid separator for separating liquid from gases, and particularly for separating liquids from expiration gases in medical analysis instruments.

When a gas sample from expiration gases is led in a patient circuit to an analysis instrument, it is unavoidable that moisture, secretion, blood, bacteria, etc., are liable to accompany the sample. As the temperature falls when the gas sample is led from the patient circuit to the analysis instrument, moisture present in the gas precipitates in the form of water droplets. Should water, blood or secretion enter the analysis instrument, there is a serious risk that the instrument will be permanently damaged, and consequently various protective solutions for preventing such contamination have been proposed in the art.

The simplest method of avoiding the ingress of bacteria, blood and secretion into the gas sample is to place a hydrophobic bacteria filter in the orifice of the sampling conduit proximal to the patient circuit. One drawback with this solution resides in the difficulty of obtaining a filter surface, which is sufficiently large to prevent the rise time of the gas measuring process from being impaired. A filter that has a small surface area will quickly become blocked and there-with result in an interruption in the gas monitoring process.

The presence of a bacteria filter in the orifice of the sampling conduit will not solve the moisture problem, because the moisture does not precipitate from the sample until the

sample is downstream of the filter. One solution to this problem is to use a special hose material, Nafion®, which allows moisture to wander freely through the hose wall. This material, however, is very expensive which makes it difficult
5 to obtain viable products when using said material.

Alternatively, water droplets, and possibly also secretion, can be separated from expiration gas in a water trap. A positive, inexpensive and effective separator can be obtained, by
10 combining the water trap with a bacteria filter. However, one drawback with this solution is that the rise time of the gas measuring process will be seriously impaired unless the water trap is adapted with respect to the volume of gas that shall be processed at that particular time.

15 The need for a short rise time is particularly accentuated when measuring the expiration gas of newly born infants, e.g. neonatal patients. Small children usually have a considerably higher respiration rate than adults. 40-60 breaths per minute
20 is normal for such infants, as compared to about 12 breaths per minute for adults. Thus, in this case the gas sampling system must have a pneumatic rise time of well above 0.5 s in order to carry out a correct gas analysis with respect to time, a rise time of 200 ms being an appropriate value in
25 this respect.

The pneumatic rise time of the gas sampling system is essentially inversely proportional to the sampling flow, in other words a high rate of flow results in a short rise time. Respiration volumes of several litres are normal in the case of
30 adult patients, which enables sample flow rates in the order of 200-300 ml/min to be used without influencing the respiratory circuit. However, in the case of neonatal patients,

which have respiratory volumes in the order of decilitres, it is necessary to lower the rate of flow to a minimum. 50 ml/min is a normal flow rate in this latter case. Consequently, when the need for a short rise time is greatest, the possibilities of achieving such a rise time are the worst.

In addition to needing to extract moisture, bacteria, etc., from the expiration gas of a patient, it is also necessary to protect the analysis instrument from dirt and other contaminants present in the ambient air. Many gas analysis instruments have long warm-up times, meaning that the instrument is normally never switched off. Consequently, if the instrument is left switched on for a long period of time in the absence of a protective filter, the measuring chamber of the analyser will gradually become dirty with progressively poorer performances as a result.

Water traps have been the solution that has been used to increasing extents to eliminate moisture in gas samples. EP-A2-0 549 266 teaches a method of extracting both moisture and other foreign particles with the aid of a hydrophobic bacteria filter. In the case of the water trap described in this prior publication, the gas sample is passed through a passageway that is divided in an upper half and a lower half of the hydrophobic filter. The moist gas sample is led into the front edge of the lower half of a passageway and is caused to exit by applying a strong sub-pressure to an opening in the rear edge of the upper half of said passageway. The liquid extracted by this arrangement is led away by applying a weak sub-pressure to an opening in the rear edge of the lower half of the passageway.

One drawback with this known water trap is that it requires a relatively large filter area, about 1 cm², in order to ensure that the product will have a sufficient length of life. The length of the passageway is limited chiefly by the desire to obtain the smallest possible unit. A length of about 3.5 cm has been found suitable. Consequently, a passageway diameter of about 3 mm is needed in order to obtain an effective filter surface. Hoses used for gas sampling purposes, however, will normally have an inner diameter of about 1.4-1.5 mm, meaning that eddy currents are generated and impaired rise time obtained when the gas sample reaches the larger diameter of the passageway.

Accordingly, the object of the present invention is to provide a liquid separator that avoids the aforesaid drawback with the earlier known water trap.

This object is achieved with an inventive liquid separator that has the characteristic features set forth in the accompanying Claims.

There is provided in accordance with the invention a liquid separator for extracting liquid from gases, said separator comprising a water trap that includes a container, a connection for incoming gas flows, a separation chamber that includes a filter, and at least one connection passageway for conducting separated gas to an analysis instrument, wherein the water trap can be attached removably to a holder unit connected to the analysis instrument, and wherein the holder unit includes connection means for connection of the connecting passageway.

The invention also enables water traps of different sizes to be used for adults and for children, with automatic switching of the analysis instrument in accordance with the size of water trap used.

5

The invention will now be described with reference to a non-limiting exemplifying embodiment thereof and also with reference to the accompanying drawings, in which Fig. 1 is a perspective view of an inventive liquid separator, showing the water trap and the holder unit separated from one another; Fig. 2 is a perspective exploded view of the water trap shown in Fig. 1; and Fig. 3 is a perspective exploded view of the holder unit shown in Fig. 1.

15 The inventive liquid separator comprises two main parts in the form of a water trap 1 and a holder unit 2. The holder unit 2 is a part that can normally be firmly fitted to the instrument (not shown) used to analyse expiration gas. The water trap 1 is a disposable product that is preferably found in two different sizes or two different designs, one for adult patients and one for neonatal patients.

The water trap 1 includes a container 3 located beneath a separation chamber 4 provided with a connection 5 for receiving a gas flow incoming from the patient. The separation chamber includes a liquid passageway 6 and a filter 7 positioned above said passageway, for instance a bacteria filter. Located above the separation chamber 4 and connecting to the other side of the filter 7 is an upper chamber part 8 that includes a gas passageway (not shown) corresponding to the liquid passageway 6 in the separation chamber and leading to connection passageways 9, 10 by means of which the water trap can be connected to the holder unit 2 and to the analysis

instrument respectively. The upper chamber part 8 is covered by a hood or cap 11. The separation chamber 4 is fitted externally with locking tabs 12 which enable the water trap 1 to be snapped firmly to the holder unit 2.

5

The separation chamber 4 is preferably fixed permanently to the upper chamber part 8, for instance ultrasound welded thereto. The filter 7, which is inserted between the separation chamber and the upper chamber part 8, may be of the PTFE
10 kind and has a pore size of about 0.5 μm and may be sealed with the aid of a labyrinth seal formed in the separation chamber and the upper chamber part. The container 3 of the water trap is adapted so as to be removable from the separation chamber 4 and therewith enable liquid collected in the
15 container to be emptied therefrom.

The holder unit 2 includes a cavity 13 in which part of the water trap 1 can be accommodated. The holder unit includes locking apertures 14 which receive the locking tabs 12 on the
20 water trap and therewith lock the trap 1 firmly in the holder unit. Two connection devices 15, 16 are provided behind the cavity 13 for receiving the connection passageways of the water trap 1. These connection devices 15, 16 are connected to hoses passing to the analysis instrument. Two electric
25 contact elements 17, 18 are provided in the rear edge of the cavity 13 and are activated by insertion of a water trap 1 into the cavity 13 of the holder unit 2.

The electric contact elements 17, 18 are adapted so that one
30 contact element will detect the presence of a water trap in the holder unit, wherewith when the water trap 1 is removed from the holder unit 2 the contact element will function to immediately stop the flow to the analysis instrument, or will

stop said flow after a certain time delay, so that no air and possible contaminants will be sucked into the instrument and contaminate the same. The other electric contact element is adapted to detect the type of water trap inserted into the holder unit. The two different types of water trap mentioned above may be designed differently at the contact region with said other electric contact element, for instance such that when using a water trap intended for children the contact will be pressed in, while providing a water trap intended for adult patients with an aperture which will mean that said other electric contact will not be pressed in when fitting said trap. The second electric contact element will then be arranged so that when it is pressed-in by fitting a water trap intended for neonatal patients, the analysis instrument will be switched to a mode in which it operates with a lower rate of flow.

The two connection passageways 9, 10 are connected to the connection devices 15, 16 of the holder unit 2 so that both a main flow that passes from the water trap to the analysis instrument and a secondary flow that passes through the container of the water trap can be obtained.

The main difference between the two water trap embodiments is that one is intended for adult patients and has a passageway width of about 3 mm, whereas the neonatal model has a passageway width of about 1.4 mm. The smaller passageway width in the neonatal model means that the rise time will be much quicker than in the case of the adult model. In this case, the problems normally occurring with shorter product life lengths are compensated for by using a lower rate of sample flow.

Because the type of water trap used can be identified, the analysis instrument can be set automatically to choose an optimal rate of sample flow for respective models through the medium of said electric contact elements. In the case of the
5 adult model, there is normally used a flow rate in the order of 200-300 ml/min, whereas a flow rate of about 50 ml/min is normally used in the case of the neonatal model. Switching between these flow rates can thus take place fully automatically, without the risk of a wrong setting being made manu-
10 ally.

CLAIMS

1. A liquid separator for separating liquid from gases and comprising a water trap (1) that includes a container (3), a connection (5) for incoming gas flow, a separation chamber (4) that includes a filter (7), and at least one connection passageway (9, 10) for leading liquid-free gas to an analysis instrument, characterised in that the water trap (1) can be removably fitted in a holder unit (2) connected to the analysis instrument; and in that the holder unit (2) is provided with connection devices (15, 16) for accommodating the connection passageway (9, 10).

2. A liquid separator according to Claim 1, characterised in that the connection device (15, 16) is a quick-fastener device for connection to the connection passageway (9, 10).

3. A liquid separator according to Claims 1 and 2, characterised in that the water trap (1) includes two connection passageways (9, 10), and in that the holder unit (2) includes two connection devices (15, 16).

4. A liquid separator according to any one of the preceding Claims, characterised in that the holder unit (2) includes a first electric contact element (18) which functions to detect the presence of a liquid trap (1) in the holder unit and to stop the flow of sample gas to the analysis instrument when no water trap is fitted in the holder unit.

5. A liquid separator according to any one of the preceding Claims, characterised in that the holder unit (2) includes a second electric contact element (17) which functions to detect the type of water trap (1) fitted in the holder unit and

to adjust the analysis instrument in accordance with the type of water trap used.

6. A liquid separator according to Claim 5, characterised in
5 that the water trap (1) is designed in different sizes for infants and adults; and in that one size includes means for actuating the second electric contact element (17) of the holder unit.
- 10 7. A liquid separator according to any one of the preceding Claims, characterised in that the water trap (1) is intended for one-time use only.

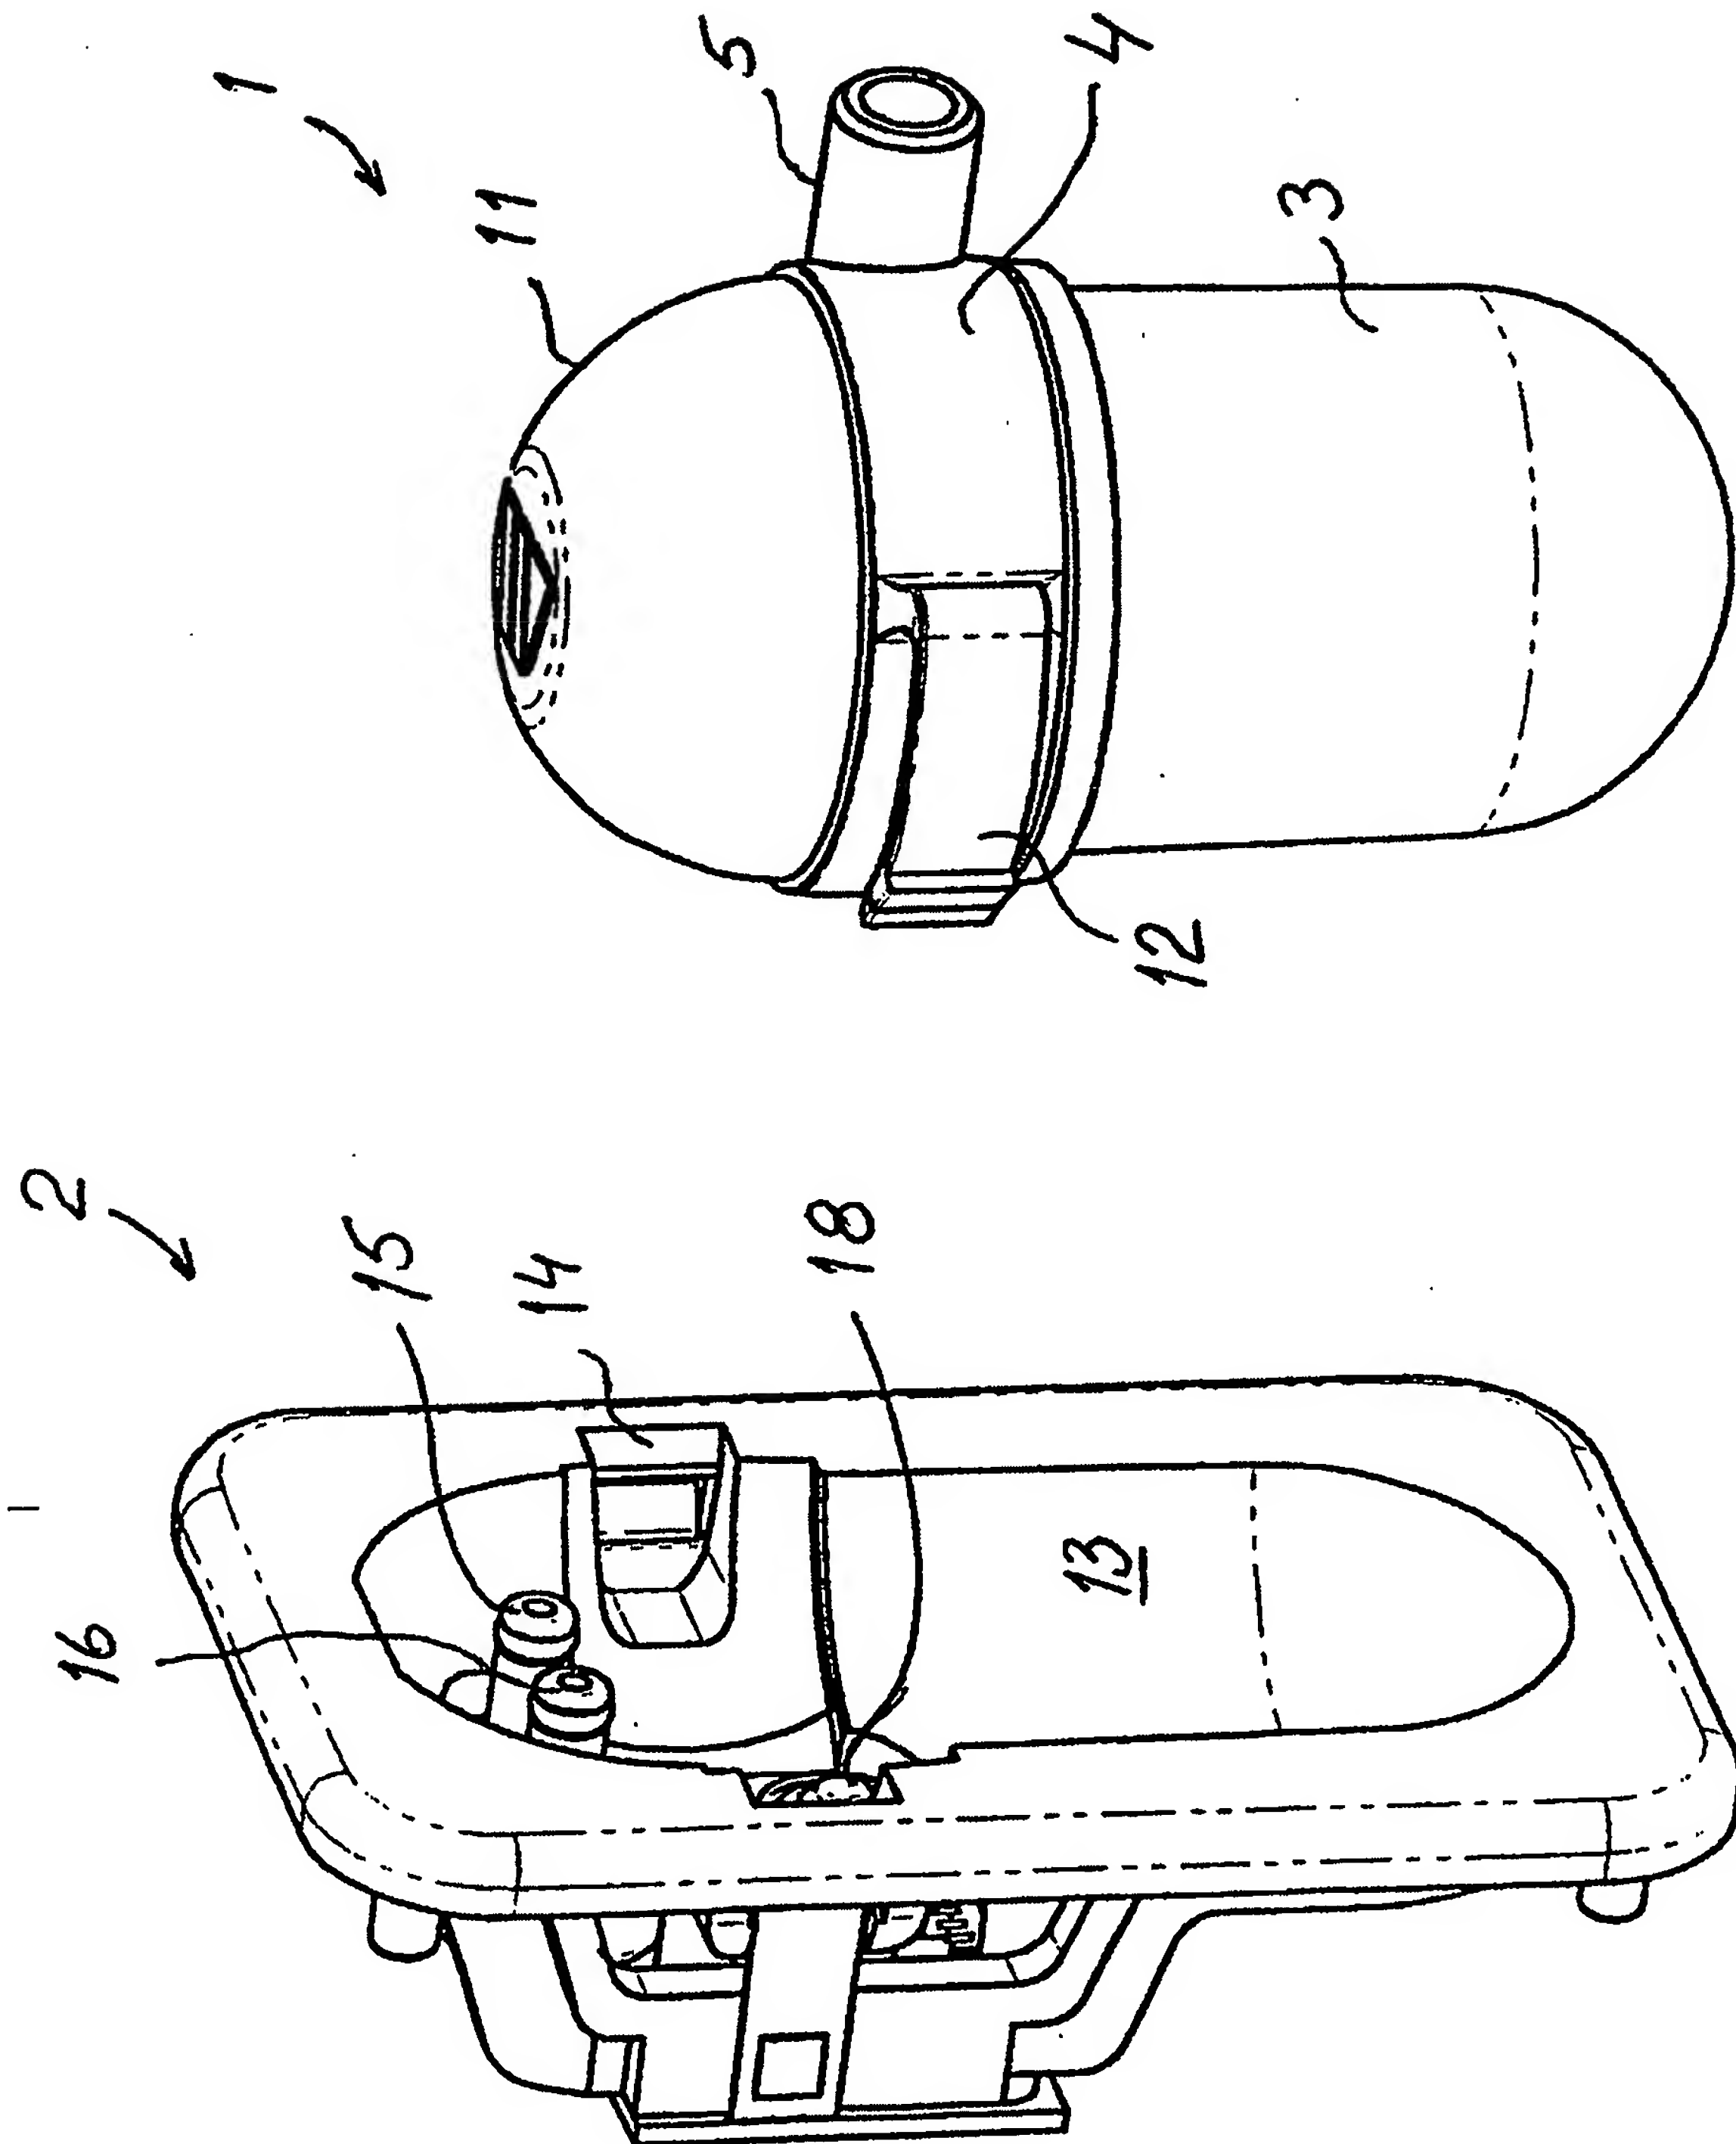


Fig. 1


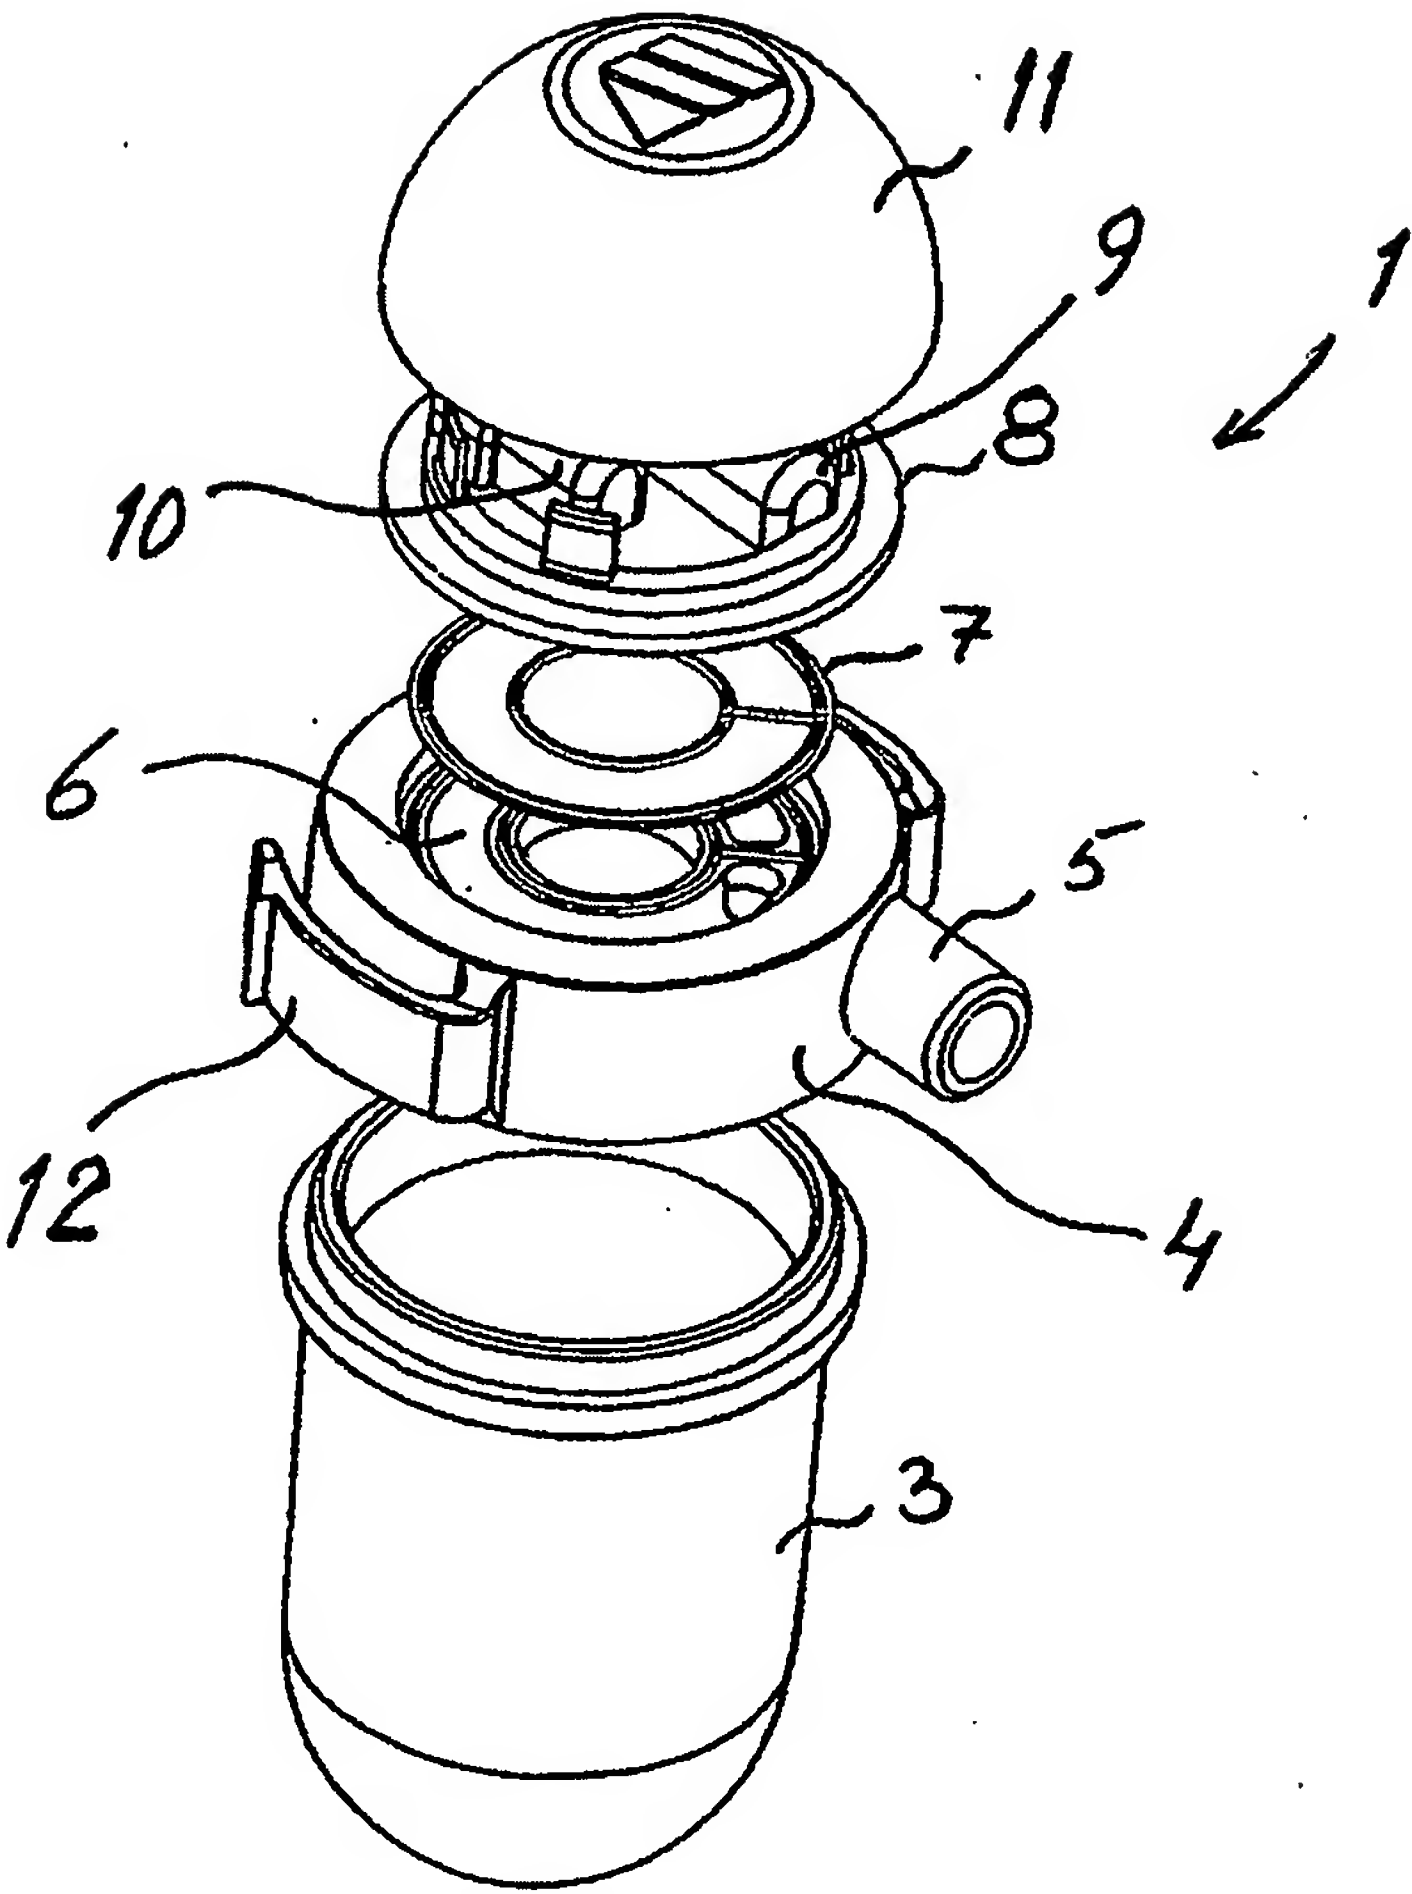


Fig. 2

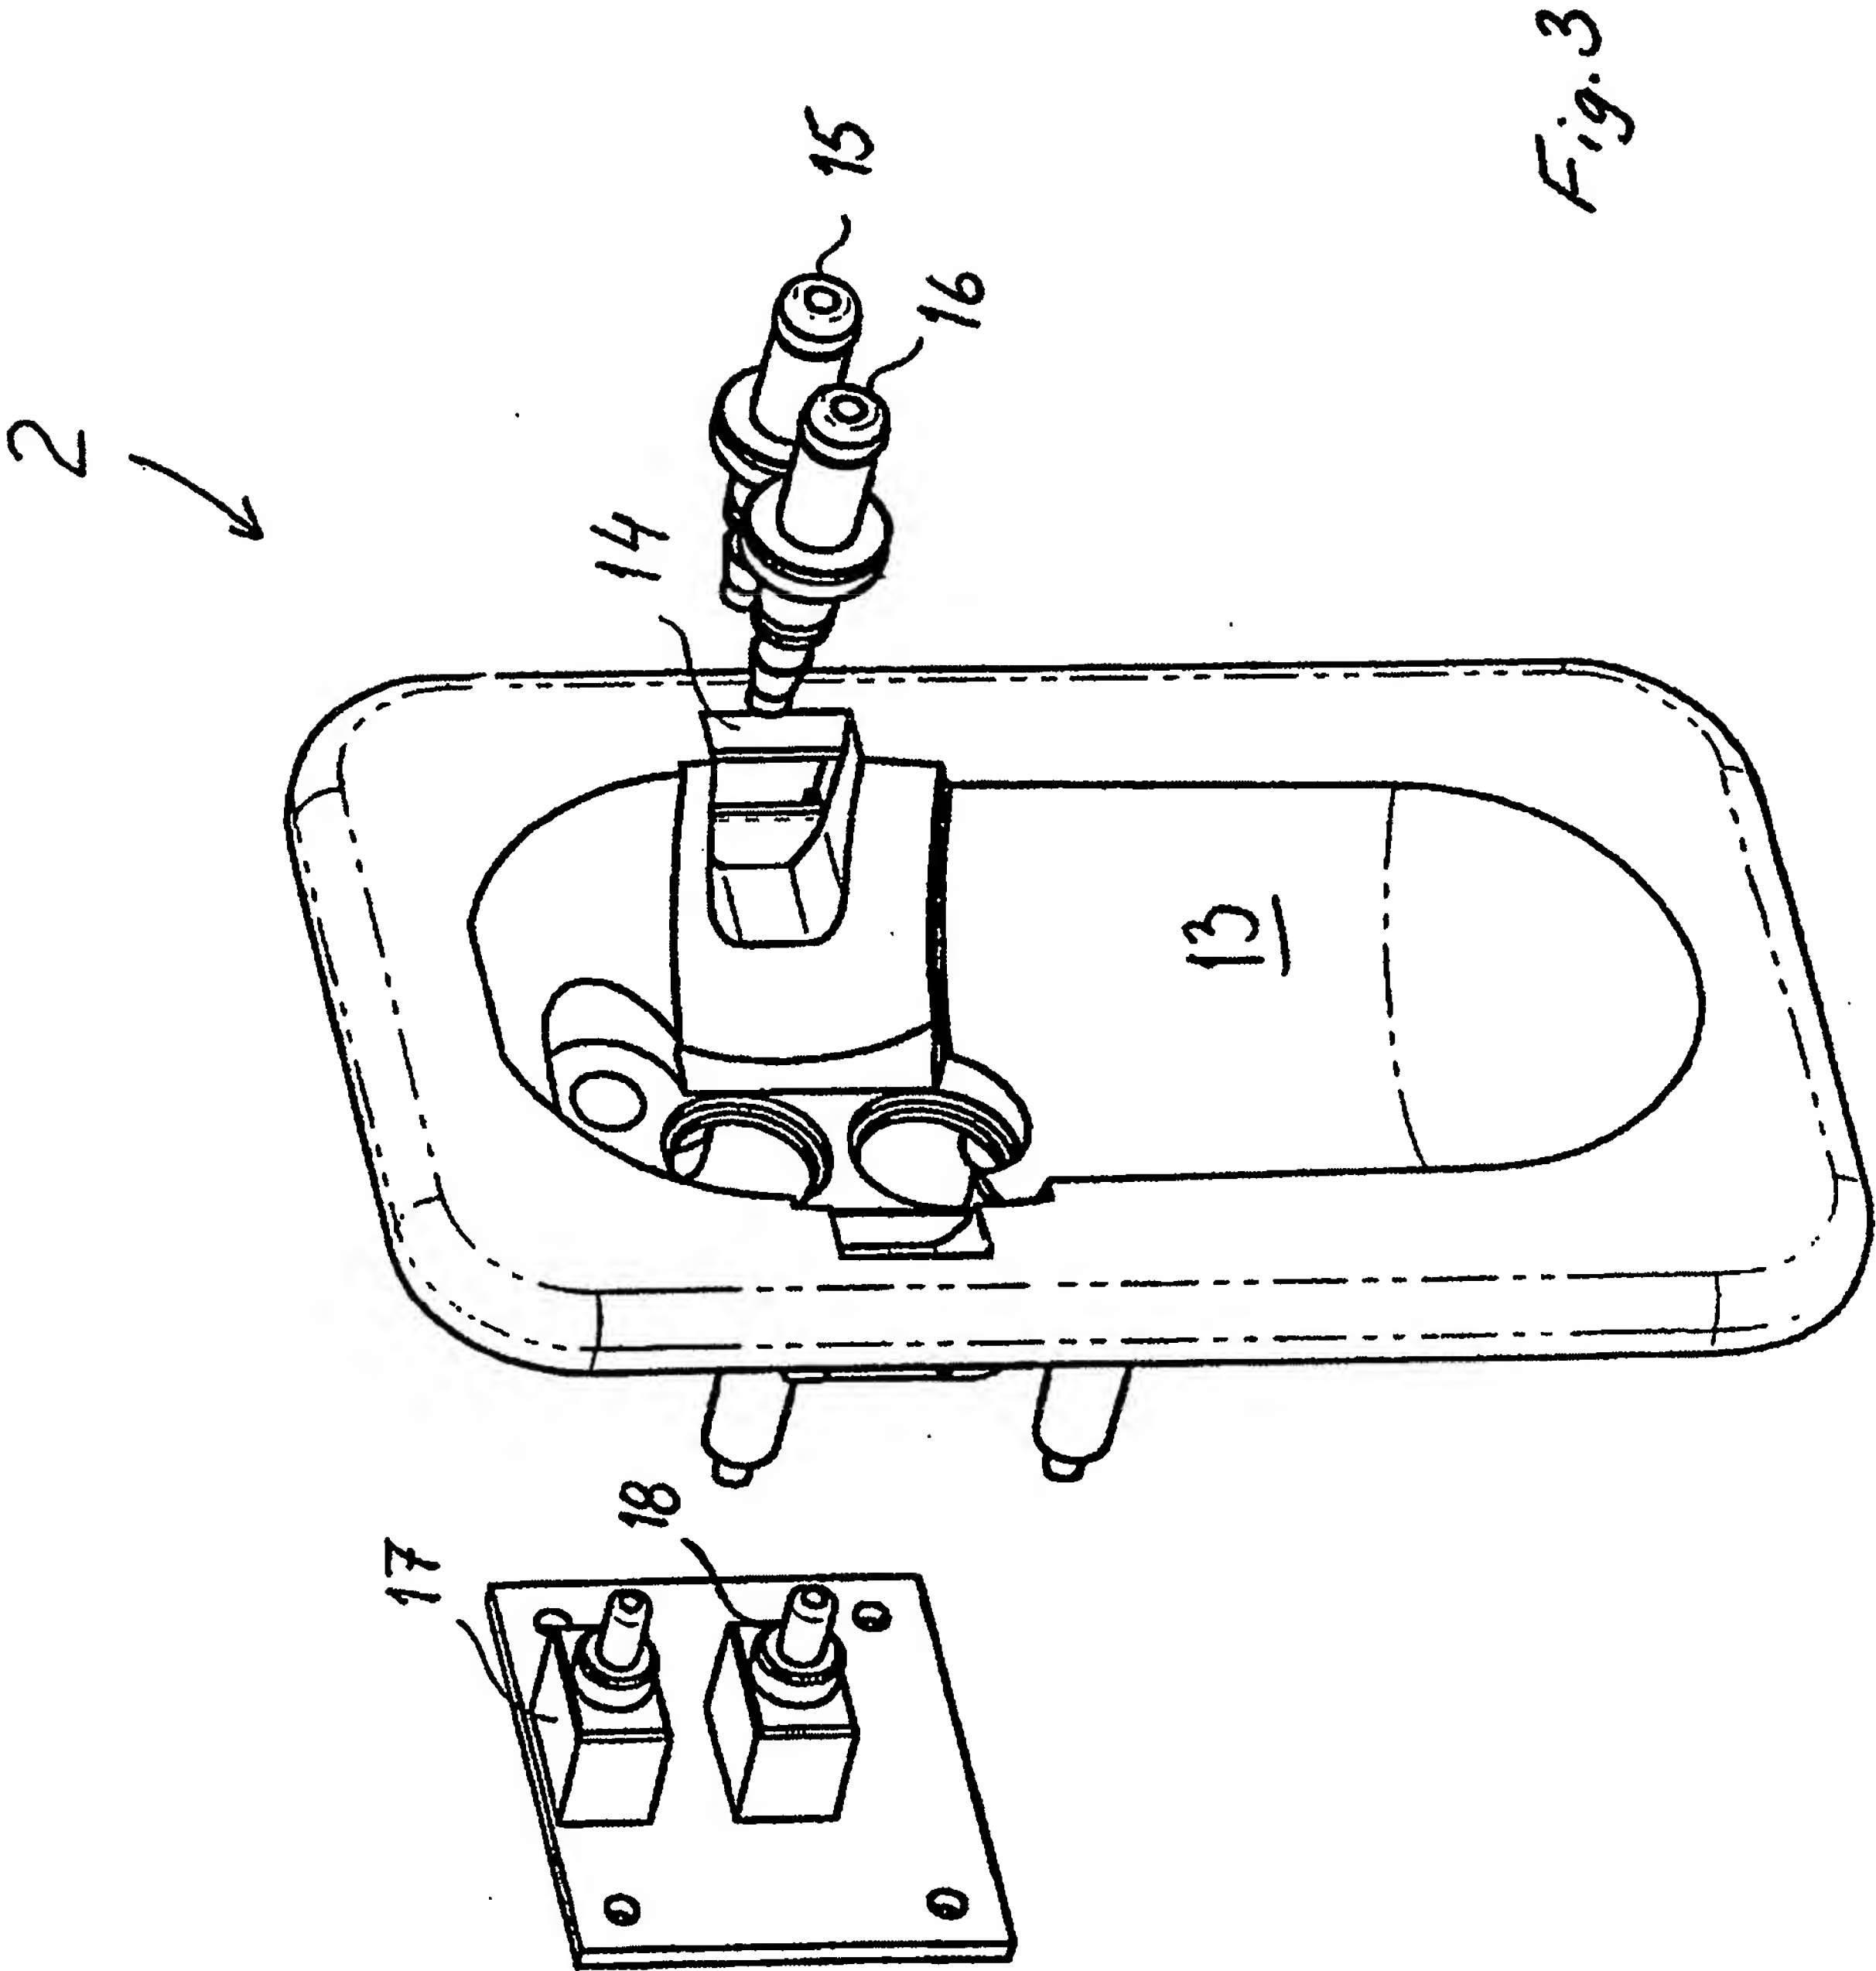

INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/00113

A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61M 16/08, A61B 5/08

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61B, A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 0242790 A2 (SPACELABS, INC.), 28 October 1987 (28.10.87), page 1, line 28 - page 2, line 9; page 4, line 20 - line 26, figure 3 --	1-7
A	EP 0549266 A2 (INSTRUMENTARIUM CORPORATION), 30 June 1993 (30.06.93), figure 2, abstract -- -----	1-7

☐ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

16 June 2000

Date of mailing of the international search report

26-06-2000

Name and mailing address of the ISA/

Swedish Patent Office

Box 5055 S-102 12 STOCKHOLM

Authorized officer

Gilla Lückman/AF

INTERNATIONAL SEARCH REPORT
Information on patent family members

02/12/99

International application No.
PCT/SE 00/00113

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 0242790 A2	28/10/87	AT 72951 T CA 1302304 A DE 3776948 A JP 63023643 A US 4717403 A	15/03/92 02/06/92 09/04/92 30/01/88 05/01/88
EP 0549266 A2	30/06/93	FI 92138 B,C FI 916041 A US 5365938 A	30/06/94 21/06/93 22/11/94